



Applicant: Mark Ealey
Serial No.: 10/730,514
Title: TRANSVERSE ELECTRODISPLACIVE
ACTUATOR ARRAY
Docket No.: XIN-102J
Attorney: Roy J. Coleman, Reg. No. 48,863

REPLACEMENT SHEET 1/8

1/8

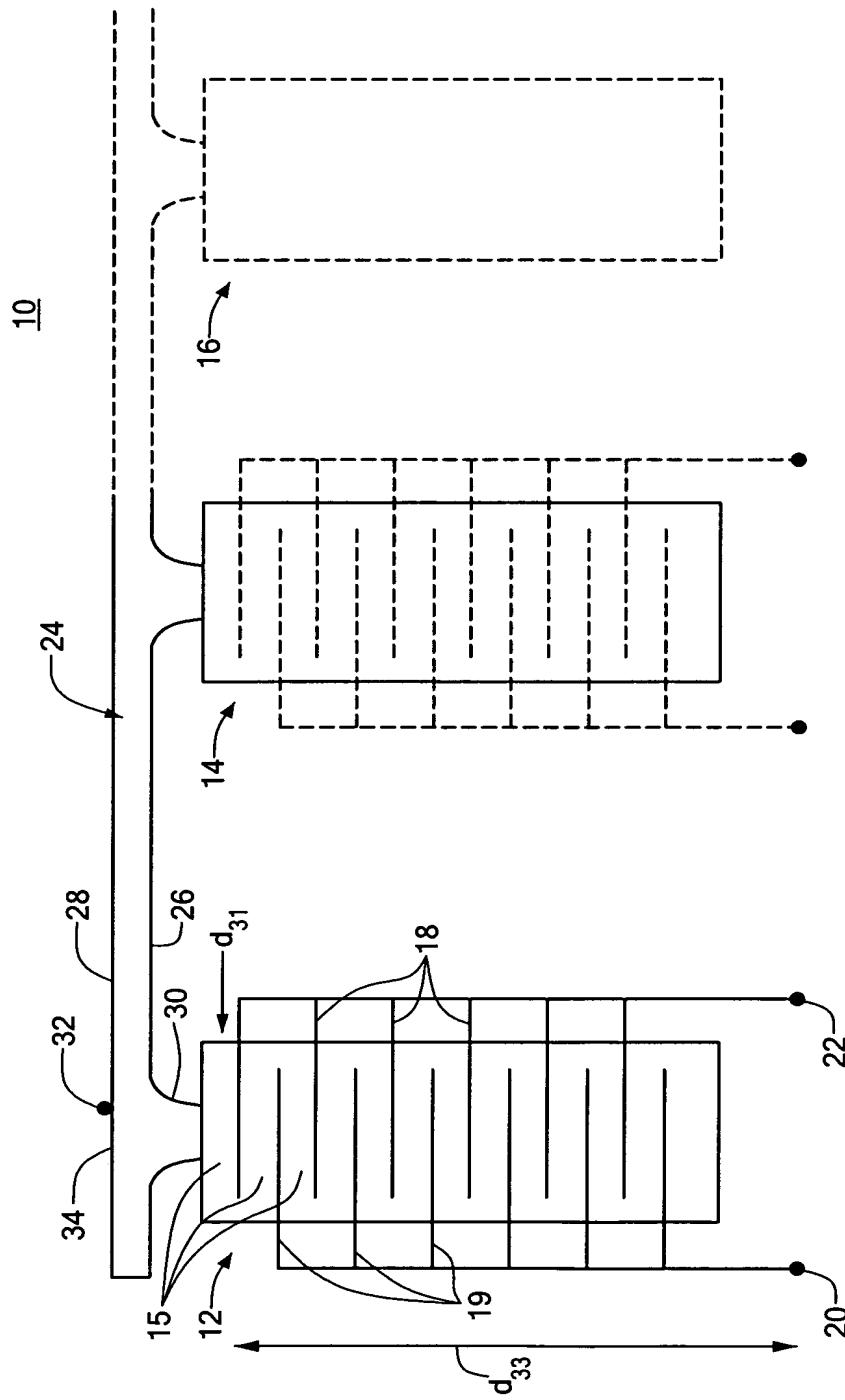


FIG. 1

PRIOR ART

REPLACEMENT SHEET 2/8

2/8

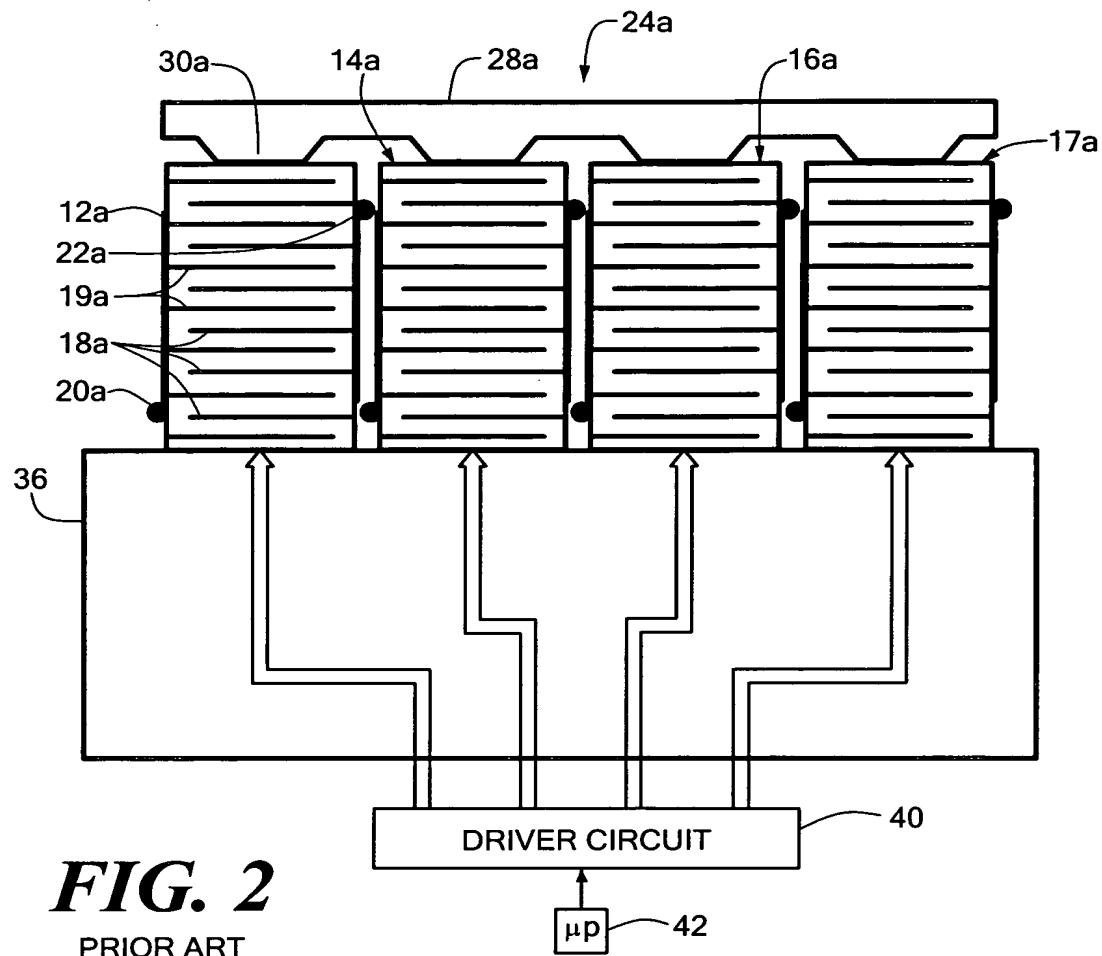


FIG. 2
PRIOR ART

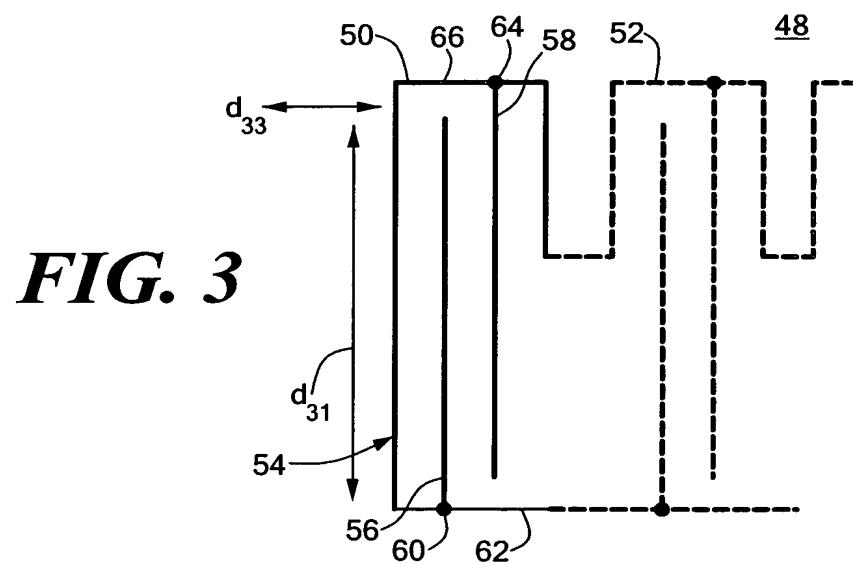


FIG. 3